



BLACK
FOREST
MEDICAL
GROUP

DORO®

CRANIAL STABILIZATION & RETRACTOR SYSTEMS



CREATE A NEW WORLD IN NEUROSURGERY WITH US!

Each neurosurgical intervention means a new challenge. Every minute counts. Every step needs to fit. A smooth workflow is essential. The Black Forest Medical Group is proud to support you and your team with innovative solutions that make neurosurgical interventions safer and more efficient.

From our history to the present and turning into the future, we were and always will be driven by the desire to satisfy your needs. Together, we are able to multiply our strengths, making a lasting difference for the health of people worldwide.



Matthias Schüle
Owner & Managing Director



Get connected





CONTENTS

RIGID & NON-INVASIVE HEADREST SYSTEMS

DORO® QR3 Headrest System	page 6
DORO® QR3 Skull Clamp	page 7
DORO® Base Units & Base Unit Parkbench	page 8
DORO® Swivel Adaptors	page 9
DORO® Crossbar Adaptor	page 9
DORO® OR Table Adaptors	page 10
DORO® Navigation Adaptors	page 10
DORO® Skull Pins	page 11
DORO® QR3 Headrest System Teflon®	page 12
DORO® Horseshoe Headrests Aluminum	page 13
DORO® Accessories	page 13
DORO® Multi-Purpose Skull Clamp	page 14

IMAGING SOLUTIONS

DORO LUCENT® Headrest System	page 20
DORO® Skull Clamp Radiolucent	page 21
DORO LUCENT® Navigation Adaptors	page 22
DORO LUCENT® Accessories	page 22
DORO® Mix & Match	page 23
DORO® Horseshoe Headrests Radiolucent	page 24
DORO LUCENT® Horseshoe Headrest ENT	page 25
DORO® QR3 XTom Headrest System	page 26
DORO LUCENT® iMRI Headrest Systems	page 28
DORO LUCENT® iXI Headrest System	page 30
DORO LUCENT® Product Trainings	page 34
DORO LUCENT® iMRI & iXI Accessories	page 34
DORO® Skull Clamp for Spinal Frames	page 35
DORO® OR Table Adaptors Radiolucent	page 36

RETRACTOR SYSTEMS

DORO LUNA® Retractor System	page 40
DORO COBRA® Retractor System	page 42
DORO® Mix & Match	page 43
DORO® Flexible Rotary Arms	page 44
DORO® Quick-Clamp Radiolucent	page 45
DORO® Halo Retractor System	page 46
DORO® Retractor Accessories	page 47
DORO® Sterilization Trays	page 47
DORO® Micro Blades	page 48
DORO® Blades	page 49





CRANIAL STABILIZATION

Rigid & Non-Invasive Headrest Systems

Firm positioning of the cranium is essential during neurosurgical procedures for patient safety and the overall outcome of the surgical approach, especially when using technologies like microscopes or navigation. We are driven to create solutions which ensure stability and safety, and provide the strength and flexibility to perform at your very best - whatever your next case might be.

DORO® QR3 HEADREST SYSTEM

The DORO® QR3 Headrest System is developed for daily use in non-imaging neurosurgical applications. Features like built-in navigation adaptor interfaces and Mix & Match compatibility with DORO® Radiolucent products make it a time-saving and versatile device.

DORO® QR3 Headrest System

Item no. 1001.100
(shown with DORO® Skull Pins)

Included Items	Item no.
DORO® QR3 Skull Clamp	1001.001
DORO® Swivel Adaptor Aluminum	3002-00
DORO® Base Unit Aluminum	3001-00



DORO® Storage Case Headrest System

Item no. 1001.030
(optionally available).

VERSATILE

With the DORO® QR3 Skull Clamp as a basis, you are free to enhance the set-up to what suits you best. Retractor arms, entire retractor systems or navigation adaptors – it all fits.

INTUITIVE

Fast and easy mounting frees up resources for the rest of your surgery preparations.

COMPATIBLE

Can directly be attached to an OR table via the neuro interface or mounted to its side-rails utilizing DORO® Side Rail Adaptors (page 10). You can also Mix & Match it with radiolucent DORO® products (page 23).



DORO® QR3 Headrest System
Item no. 1001.100

DORO® QR3 SKULL CLAMP

REDUCED RISK OF LACERATIONS

No play between archholder and skull base when locked.

EASY TO READ PRESSURE SCALE

Metric and imperial units.

PRECISE NAVIGATION


Navigation tracking device adaptors (page 10) can easily be attached in close proximity to the surgical field.

SPACIOUS

Due to its unique shape there is always free space to place the intubation tube, even in prone position.

EASY, SAFE AND STABLE INTERFACE

Attach DORO LUNA®, DORO COBRA® or Quick-Clamp products to the form-fitting Quick-Rail® interface (Infobox below).

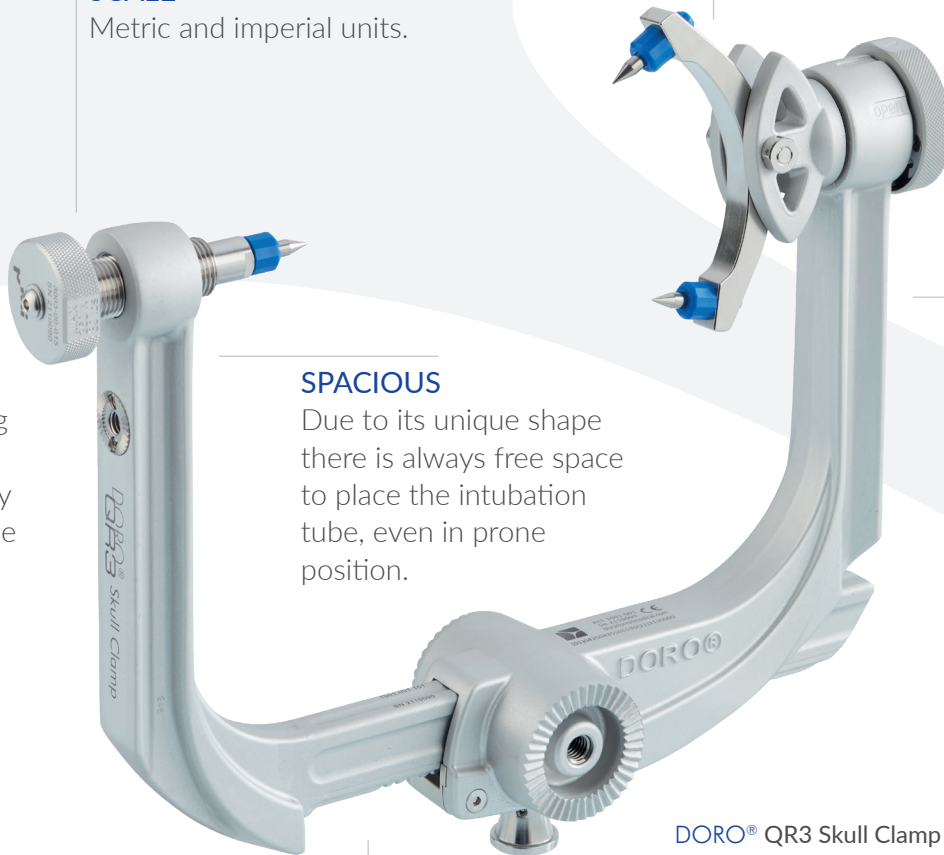

DORO® QR3 Skull Clamp
Item no. 1001.001

STABLE

Minimum play between the skull clamp base and the extension arm ensures high stability and a reduced risk to lost navigation.



QUICK-RAIL® AN INNOVATIVE INTERFACE


The term QR3 refers to the 3rd generation of our innovative Quick-Rail® technology which is directly implemented in the extension arms of our aluminum skull clamps. Due to its unique shape it can easily be located, even when covered by multiple layers of sterile drape. The Quick-Rail® serves as a form-fitting interface, ensuring reliable attachment of DORO® Retractor Systems and accessories.

DORO® ALUMINUM BASE UNITS


DORO® Base Units are individually designed for specific OR tables. Additionally, you can attach DORO® Base Units to virtually any common OR table with DORO® Side Rail OR Table Adaptors (page 10).




DORO® Adjustable Base Unit
Item no. 3001-00

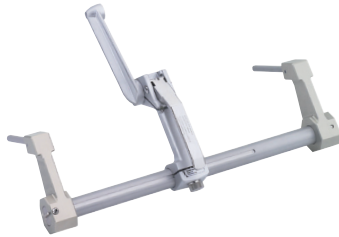

DORO® Adjustable Base Unit
Mizuho
Item no. 3001-002

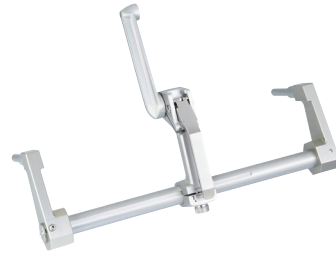

DORO® Adjustable Base Unit
Takara Belmont
Item no. 3001-001

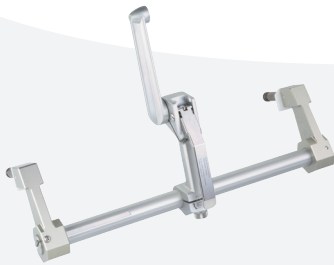


DORO® Adjustable Base Unit
Eschmann T-Series
Item no. 3001-010

DORO® BASE UNIT PARKBENCH

The DORO® Base Unit Parkbench is the perfect solution for lateral patient positioning. Its design allows a safe and comfortable positioning of the patient's arm, resulting in a reduced risk of hematomas. The Base Unit Parkbench is adjustable in width and attaches to almost all standard siderails.



DORO® Base Unit Parkbench
Item no. 3001-006



Universal Side Rail Fitting
Item no. 3007-50

Connects the Armrest Parkbench to the DORO® Base Unit Parkbench.



Armrest Parkbench
Item no. 3001-007

DORO® SWIVEL ADAPTORS

DORO® Swivel Adaptors are the connecting elements between DORO® Skull Clamps and DORO® Base Units. Versions offering pivoting features and additional starbursts are available.



DORO® Swivel Adaptor
Item no. 3002-00

Provides 360° rotation for optimum flexibility in patient positioning.



DORO® Swivel Adaptor Navigation
Item no. 3002-60

Provides 360° rotation and two additional starbursts for increased options in mounting navigational or similar devices.

DORO® CROSSBAR ADAPTOR

The DORO® Crossbar Adaptor is the perfect solution for all approaches requiring the patient to be in sitting position. It can be mounted to the side-rails of virtually any standard OR tables and provides a stable interface for the DORO® QR3 Headrest System.



DORO® Crossbar Adaptor
Item no. 3007-00

Needs 2x Universal Side Rail Fittings (item no. 3007-50, see page 8).



DORO® ALUMINUM OR TABLE ADAPTORS




DORO® Table Adaptor
Item no. 3010-00

Mounted on square receptacle of OR table.



DORO® Side Rail OR Table Adaptor
Item no. 3011-00

Width-adjustable universal neuro interface, fitting OR tables with bars up to 70 mm.

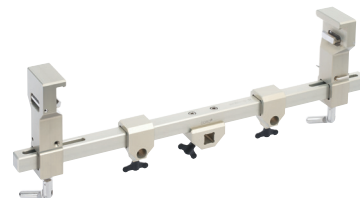

DORO® Side Rail OR Table Adaptor AMSCO®
Item no. 3011-10

Width-adjustable universal neuro interface, fitting OR tables with bars up to 125 mm.



AMSCO® Headrest Adaptor
Item no. 3011-11

Fits 3080 & 3085 series.

DORO® NAVIGATION ADAPTORS

DORO® Easy Connect Navigation Adaptors connect directly to the integrated navigation starburst on the Quick-Rail® of the DORO® QR3 Skull Clamp, DORO® Multi-Purpose Skull Clamp and DORO® Skull Clamp Teflon®. This provides a very stable and secure connection and allows positioning the navigation reference array close to the surgical target.



DORO® Easy Connect Navigation Adaptor Stryker®
Item no. 1204.001

(Shown with Stryker navigation reference array).



DORO® Easy Connect Navigation Adaptor Brainlab
Item no. 1204.002

(Shown with Brainlab navigation reference array).



DORO® Easy Connect Navigation Adaptor Medtronic
Item no. 1204.003

(Shown with Medtronic navigation reference array).

DORO® REUSABLE SKULL PINS



DORO® Reusable
Skull Pins
Stainless Steel
Adult
Color: Black
Item no. 3005-00
(3 pins)



DORO® Reusable
Skull Pins
Stainless Steel
Pediatric
Color: Black
Item no. 3004-00
(3 pins)



DORO® Reusable
Skull Pins
Titanium
Adult
Color: Blue
Item no. 3005-50
(3 pins)



DORO® Reusable
Skull Pins
Titanium
Pediatric
Color: Blue
Item no. 3004-50
(3 pins)

DORO® DISPOSABLE SKULL PINS



DORO® Disposable
Skull Pins
Stainless Steel
Adult
Color: Blue
Item no. 3006-00
(36 pins), sterile



DORO® Disposable
Skull Pins
Stainless Steel
Pediatric
Color: Yellow
Item no. 3006-10
(36 pins), sterile




DORO® Disposable
Skull Pins
Titanium
Adult
Color: Orange
Item no. 3006-20
(36 pins), sterile



DORO® Disposable
Skull Pins
Titanium
Pediatric
Color: Green
Item no. 3006-30
(36 pins), sterile



DORO® Disposable
Skull Pins
Stainless Steel
Adult
Color: Black
Item no. 3006-50
(36 pins), sterile

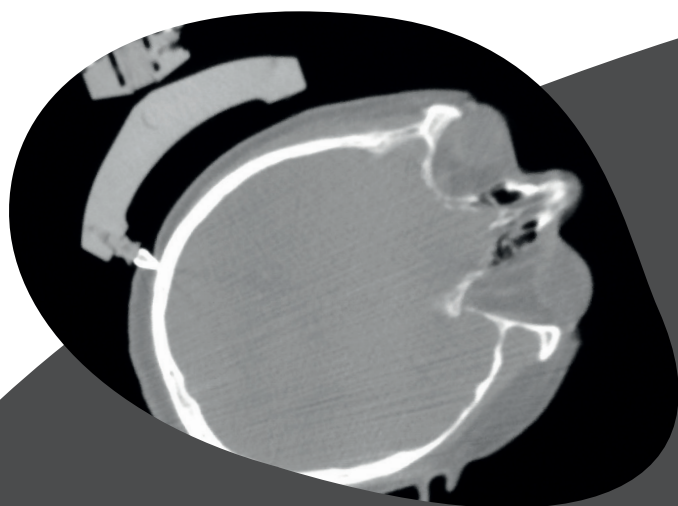

HIGH-END IMAGING

Perfect balance of imaging quality and pin stability. The DORO LUCENT® Disposable Skull Pin is specifically designed for intra-operative imaging applications using CT, MRI, X-Ray and Fluoroscopy. Imaging artifacts are reduced to a minimum while the composition of a titanium tip and high-performance reinforced polymer ensures a precise, secure and rigid fixation of the patient's head.



DORO LUCENT® Disposable Skull Pins

Adult, sterile

Color: Black

Item no. 1106.003 (3 pins) (Not available in the USA & Canada.)

Item no. 1106.103 (9 pins)

DORO® QR3 HEADREST SYSTEM TEFLON®

The DORO® QR3 Headrest System Teflon® is the sterilizable counterpart of our well-established DORO® Headrest System Aluminum. Its autoclavability is a major plus when you are treating highly infectious patients.

DORO® QR3 Headrest System Teflon®

Item no. 3003-100
(shown with DORO® Skull Pins)

Included Items	Item no
DORO® Skull Clamp Teflon®	3003-009
DORO® Swivel Adaptor Teflon®	3002-009
DORO® Adjustable Base Unit Teflon®	3001-009

PRECISE NAVIGATION

Navigation tracking device adaptors (page 10) can easily be attached closely to the surgical field.

EASY, SAFE AND STABLE CONNECTION

Attach DORO LUNA®, DORO COBRA® or Quick-Clamp products to the form-fitting Quick-Rail® interface.

AUTOCLAVABLE

The Teflon® coated surface of the DORO® QR3 Headrest System Teflon® makes it machine-washable and autoclavable.

It conforms to World Health Organization (WHO) Infection Control Guidelines for cleaning and sterilization.



DORO® Storage Case Headrest System
Item no. 1001.030
(optionally available).



DORO® QR3 Headrest System Teflon®
Item no. 3003-100

DORO® HORSESHOE HEADREST ALUMINUM



SKELETAL TRACTION OPTION

DORO® Horseshoe Headrests Aluminum are available with or without an Extension Bar.

PROPER PATIENT POSITIONING

All DORO® Horseshoe Headrests are adjustable in width.

ONE BASE FITS ALL

Mount adult or pediatric gel pads to the same horseshoe base.

ADULT VERSION

DORO® Swivel Horseshoe Headrest System, Adult with Extension Bar

Item no. 3009-00

Included Items	Item no.
DORO® Horseshoe Base	3009-01
DORO® Horseshoe Pad, Adult, right	3009-10
DORO® Horseshoe Pad, Adult, left	3009-11
DORO® Extension Bar Horseshoe	3009-25

DORO® Swivel Horseshoe Headrest System, Adult without Extension Bar

Item no. 3009-02

Included Items	Item no.
DORO® Horseshoe Base	3009-01
DORO® Horseshoe Pad, Adult, right	3009-10
DORO® Horseshoe Pad, Adult, left	3009-11

PEDIATRIC VERSION

DORO® Swivel Horseshoe Headrest System, Pediatric with Extension Bar

Item no. 3008-00

Included Items	Item no.
DORO® Horseshoe Base	3009-01
DORO® Horseshoe Pad, Pediatric, right	3008-10
DORO® Horseshoe Pad, Pediatric, left	3008-11
DORO® Extension Bar Horseshoe	3009-25

DORO® Swivel Horseshoe Headrest System, Pediatric without Extension Bar

Item no. 3008-02

Included Items	Item no.
DORO® Horseshoe Base	3009-01
DORO® Horseshoe Pad, Pediatric, right	3008-10
DORO® Horseshoe Pad, Pediatric, left	3008-11

DORO® ACCESSORIES



DORO® Cervical Spine Support

Item no. 3012-00
Neck support for anterior spine surgery.



DORO® Headrest Wall Storage Unit

Item no. 3013-00
81 cm x 94 cm
32" w x 37" h.



DORO® Lubricant HP500

Item no. 1001.999

DORO® Lubricant HP500 6-pack

Item no. 1001.998

Autoclavable and precise in its application due to its needle-shaped tip.

DORO® MULTI-PURPOSE SKULL CLAMP

The DORO® Multi-Purpose Skull Clamp is our most versatile head positioning device. It offers all the beneficial features of the DORO® QR3 Skull Clamp and can be set-up for invasive or non-invasive procedures in adult as well as in pediatric cases. Since a children's skull is still growing and therefore very vulnerable, neurosurgical solutions are needed which fit their needs. The DORO® Multi-Purpose Skull Clamp provides different kinds of shapes and sizes of gel pads and pin holders. An extension bar with a force application specifically designed for pediatric cases ensures a safe immobilization of the child's head while providing additional control over the pinning force up to 90N.

FLEXIBLE 
A large variety of DORO® Gel Pads and Pin Holders is available to support optimal patient positioning (pages 16-17).

PRECISE NAVIGATION

Navigation tracking device adaptors (page 10) can easily be attached in close proximity to the surgical field.

SUPPORTS PEDIATRIC PROCEDURES

The DORO® Multi-Purpose Skull Clamp features specifically designed components like the 90 N/20 lbs Extension Bar or the head support.



DORO® Extension Bar
90 N/20 lbs
Item no. 3020-52

EXTENDABLE


The Quick-Rail® technology enables you to attach accessories and retractor systems such as the DORO LUNA® Retractor System (page 38) easily, quickly, and securely to the skull clamp.

MIX & MATCH

Combine the DORO® Multi-Purpose Skull Clamp with a radiolucent base unit and swivel adaptor (page 23).

Which DORO® Multi-Purpose Skull Clamp System works for you?

That depends on the required head positioning method. Check below for guidance. The complete system configurations can be found on the following pages.

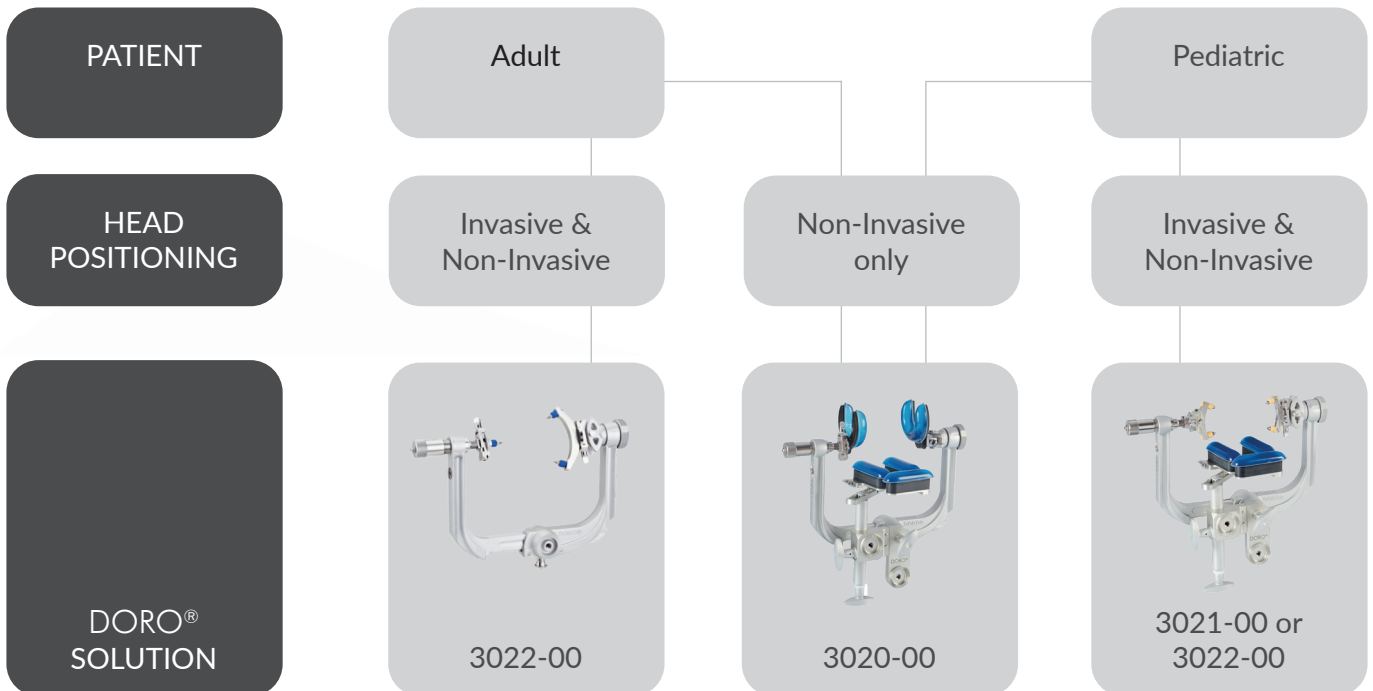

DORO® MULTI-PURPOSE – INVASIVE SET-UP

Set-up the DORO® Multi-Purpose Skull Clamp as a classic 3-pin skull clamp for adult patients or apply the dedicated 90 N /20 lbs extension bar, head support and dual pin holders on both sides when treating pediatric patients.



DORO® Abbott Multi-Purpose Skull Clamp System Pediatric

Included Items	Item no.
DORO® Disposable Skull Pins, Pediatric (36pcs)	3006-10
DORO® Pin Holder Pediatric	3020-01
DORO® Head Support (w/o Gel Pads)	3020-03
DORO® Multi-Purpose Skull Clamp	3020-50
DORO® Extension Bar 90N/20lbs	3020-52
DORO® Single Pin Holder	3020-55
DORO® Gel Head Ring w/ Base 90 mm (3pcs)	3020-61
DORO® Pin Holder Adjustable, Pediatric	3020-62
DORO® Gel Head Ring w/ Base 140 mm	3020-63
DORO® Adjustment Key	3020-65
DORO® Gel Ear Ring w/ Base 90 mm (2pcs)	3020-68
DORO® Trio Gel Pad (adjustable)	3020-71
DORO® Storage Case MPSC System	3020-001

DORO® Universal Multi-Purpose Skull Clamp System

Included Items	Item no.
DORO® Disposable Skull Pins, Adult (36pcs)	3006-00
DORO® Disposable Skull Pins, Pediatric (36pcs)	3006-10
DORO® Pin Holder Pediatric	3020-01
DORO® Gel Pad (2pcs)	3020-02
DORO® Head Support (w/o Gel Pads)	3020-03
DORO® Multi-Purpose Skull Clamp	3020-50
DORO® Extension Bar 90N/20lbs	3020-52
DORO® Single Pin Holder	3020-55
DORO® Pin Holder Adult	3020-56
DORO® Gel Head Ring w/ Base 90 mm (3pcs)	3020-61
DORO® Pin Holder Adjustable, Pediatric	3020-62
DORO® Gel Head Ring w/ Base 140 mm	3020-63
DORO® Adjustment Key	3020-65
DORO® Gel Ear Ring w/ Base 90 mm (2pcs)	3020-68
DORO® Trio Gel Pad (adjustable)	3020-71
DORO® Storage Case MPSC System	3020-001

DORO® MULTI-PURPOSE – NON-INVASIVE SET-UP

Choose from a variety of different gel pad shapes and sizes for optimal patient stabilization for non-invasive positioning. All of the pads can either be mounted to the lateral receptacles at the skull clamp or to the head support for maximized flexibility in patient positioning.



DORO® Multi-Purpose Skull Clamp
Non-Invasive Set-Up



DORO® Gel Ear Ring, with Base 90mm
Item no. 3020-68



DORO® Gel Head Ring, with Base 90mm
Item no. 3020-61



DORO® Trio Gel Pad, adjustable
Item no. 3020-71



DORO® Gel Pad
Item no. 3020-02



DORO® Gel Ear Ring, with Base 140mm
Item no. 3020-70



DORO® Gel Head Ring, with Base 140mm
Item no. 3020-63

DORO® Multi-Purpose Skull Clamp System

Item no. 3020-00

Included Items	Item no.
DORO® Disposable Skull Pins, Pediatric (36pcs)	3006-10
DORO® Pin Holder Pediatric	3020-01
DORO® Head Support (w/o Gel Pads)	3020-03
DORO® Multi-Purpose Skull Clamp	3020-50
DORO® Single Pin Holder	3020-55
DORO® Gel Head Ring w/ Base 90 mm (3pcs)	3020-61
DORO® Pin Holder Adjustable, Pediatric	3020-62
DORO® Gel Head Ring w/ Base 140 mm	3020-63
DORO® Adjustment Key	3020-65
DORO® Gel Ear Ring w/ Base 90 mm (2pcs)	3020-68
DORO® Trio Gel Pad (adjustable)	3020-71
DORO® Storage Case MPSC System	3020-001



Storage Case MPSC System
Item no. 3020-001
(shown with Multi-Purpose Skull Clamp and Accessories).

STORE IT SAFELY

All DORO® Multi-Purpose Skull Clamp systems are shipped in a protective storage case.



CRANIAL STABILIZATION

Imaging Solutions

Intra-operative imaging allows to run diagnostic imaging during surgical procedures to support decision making on how to proceed with the case at hand. Having experienced the complexity of different imaging methods and surgical approaches, we strive to provide technically advanced yet easy to use products.



DORO LUCENT® HEADREST SYSTEM

MRI CT ANGIO

The DORO LUCENT® Headrest System is the cranial stabilization system of choice for all procedures applying X-Ray & iCT Imaging. It features the completely metal free DORO® Skull Clamp Radiolucent with its beneficial Quick-Rail® interfaces for a quick and easy attachment of navigation tracking devices, retractor systems and other accessories. The DORO LUCENT® Base Unit features a completely new and streamlined design and is also available in a compact version.

DORO LUCENT® Headrest System Item no. 1101.020	
Included Items	Item no.
DORO LUCENT® Base Unit	1101.021
DORO LUCENT® Transitional Member	1101.026
DORO LUCENT® Locking Transitional Member	1101.031
DORO LUCENT® Storage Case Headrest System	1101.030
DORO LUCENT® Disposable Skull Pins, Adult	1106.003
DORO® Swivel Adaptor Radiolucent	3033-00
DORO® Skull Clamp Radiolucent	3034-00

HIGH-END IMAGING

DORO LUCENT® Disposable Skull Pins are perfectly stable and reduce imaging artifacts to a minimum (page 11).

RIGID FIXATION

Safely position the patient engaging the DORO® Skull Clamp Radiolucent.

FITTING

The system connects to virtually any OR table side-rail types.

ADAPTABLE

Compact Side Parts are additionally available.

DORO LUCENT® Headrest System
Item no. 1101.020
(shown with DORO LUCENT® Disposable Skull Pins, page 11).



SAFE

The form fitting design of the base unit provides a stable base for the entire system.

CONVENIENT HANDLING

Combined locking of transitional and sliding member.

DORO® SKULL CLAMP RADIOLUCENT

MRI CT ANGIO

**EASY TO READ
PRESSURE SCALE**
Metric and imperial
units.

**REDUCED RISK OF
LACERATIONS**
No play between archholder and
skull clamp when locked.



DORO® Skull Clamp Radiolucent
Item no. 3034-00
(shown with **DORO LUCENT®**
Disposable Skull Pins, page 11).

VERSATILE
Quick-Rail® Technology enables
you to attach accessories and
retractor systems easily, quickly,
and securely to the skull clamp.

MIX & MATCH
The **DORO®** Skull Clamp Radiolucent can
be mounted to **DORO®** Aluminum Swivel
Adaptor and Base Unit utilizing the Mix &
Match Adaptor #3033-50 (page 23).



DORO LUCENT®
Base Unit Compact
Item no. 1101.022

DORO LUCENT®
Side Part, short
Item no. 1101.038

COMPACT VERSION

Choose the **DORO LUCENT®** Headrest
System that suits you best. If you need to
keep a low profile, the **DORO LUCENT®**
Base Unit Compact offers shortened side
parts, minimizing the space between base
unit and OR table.

DORO LUCENT® NAVIGATION ADAPTORS

MRI CT ANGIO

DORO® Navigation Adaptors Radiolucent offer a safe and stable interface for navigation reference arrays from Stryker®, Medtronic and Brainlab. They are directly mounted to the Quick-Rail® of the DORO® Skull Clamp Radiolucent. These adaptors allow a close positioning of the respective navigation reference array to the patients head while keeping the sterile field intact.



DORO LUCENT®
Navigation Adaptor Brainlab
 Item no. 3033-66
 For Brainlab Reference Array 19145-01
 with or without elongation 19145-02
 (This product is not available in the USA
 & Canada.)



DORO LUCENT®
Navigation Adaptor Medtronic
 Item no. 3033-65



DORO LUCENT®
Navigation Adaptor Stryker®
 Item no. 3033-64

PLEASE NOTE:
 • Reference arrays are provided by Stryker®, Medtronic and Brainlab.

DORO LUCENT® HEADREST ACCESSORIES

MRI CT ANGIO



**DORO® Swivel Adaptor
 Radiolucent**
 Item no. 3033-00



**DORO® Swivel Adaptor
 Radiolucent, short**
 Item no. 3033-10



**DORO® Universal DRF Adaptor
 Radiolucent (includes key)**
 Item no. 3038-30



DORO LUCENT®
Storage Case Headrest System
 Item no. 1101.030



DORO LUCENT®
Locking Transitional Member
 Item no. 1101.031



DORO LUCENT®
Transitional Member
 Item no. 1101.026

MIX & MATCH



FOR CRANIAL APPLICATIONS

Mix & Match the **DORO®** Skull Clamp Radiolucent with **DORO®** Aluminum Swivel Adaptors and Base Units.



DORO® Interface Skull Clamp Radiolucent
(to ALU Swivel Adaptor)
Item no. 3033-50

FOR CRANIAL AND CERVICAL SPINE APPLICATIONS

Mix & Match the **DORO®** Radiolucent Skull Clamp and Swivel Adaptor with **DORO®** Aluminum Base Units.

DORO® Transitional Member Radiolucent (to ALU Base Unit)
Item no. 3032-00



FOR CERVICAL SPINE APPLICATIONS

Mix & Match **DORO®** Aluminum Skull Clamps with the **DORO®** Radiolucent Swivel Adaptor, Transitional Member and Base Unit.

DORO® Interface Skull Clamp Aluminum (to RDL Swivel Adaptor)
Item no. 3033-51



DORO® HORSESHOE RADIOLUCENT

MRI CT ANGIO

DORO® Radiolucent Horseshoes are the best choice for procedures that do not require a rigid fixation. The products come with an extension bar for skeletal traction. The horseshoe features a Quick-Rail® interface for the quick connection of DORO COBRA® Retractor Arms.

ADULT VERSION

DORO® Swivel Horseshoe Headrest Radiolucent Adult, with Extension Bar
Item no. 3036-00

Included Items	Item no.
DORO® Horseshoe Base Radiolucent with Extension Bar	3036-50
DORO® Horseshoe Pad, Adult, right	3009-10
DORO® Horseshoe Pad, Adult, left	3009-11

PEDIATRIC VERSION

DORO® Swivel Horseshoe Headrest Radiolucent Pediatric, with Extension Bar
Item no. 3035-00

Included Items	Item no.
DORO® Horseshoe Base Radiolucent with Extension Bar	3036-50
DORO® Horseshoe Pad, Pediatric, right	3008-10
DORO® Horseshoe Pad, Pediatric, left	3008-11



VERSATILE

Attach DORO COBRA® Retractor Arms utilizing the DORO COBRA® Quick-Clamp for Radiolucent Quick-Rail® (page 41).

DORO® HORSESHOE RS RADIOLUCENT

MRI CT ANGIO

ADULT VERSION

DORO® Horseshoe RS Headrest Radiolucent, Adult, with Extension Bar
Item no. 3036-70

Included Items	Item no.
DORO® Horseshoe RS Base Radiolucent with Extension Bar	3036-71
DORO® Horseshoe Pad, Adult, right	3009-10
DORO® Horseshoe Pad, Adult, left	3009-11

PEDIATRIC VERSION

DORO® Horseshoe RS Headrest Radiolucent, Pediatric, with Extension Bar
Item no. 3035-70

Included Items	Item no.
DORO® Horseshoe RS Base Radiolucent with Extension Bar	3036-71
DORO® Horseshoe Pad, Pediatric, right	3008-10
DORO® Horseshoe Pad, Pediatric, left	3008-11



COMPACT

Connect the Horseshoe RS directly to the DORO LUCENT® Transitional Member and benefit from a low profile.

DORO LUCENT® HORSESHOE ENT

MRI CT ANGIO

The **DORO LUCENT®** Horseshoe Headrest ENT is designed to match the specific needs of patient positioning for ear, nose and throat procedures. You can directly mount it to the **DORO LUCENT®** Transitional Member which allows a low profile by having the open part of the horseshoe facing away from the OR table.



ADULT VERSION

DORO LUCENT® Horseshoe Headrest ENT, Adult
Item no. 1101.007

Included Items	Item no.
DORO LUCENT® Horseshoe Headrest ENT, RDL w/o Gel Pads	1101.006
DORO® Horseshoe Pad, Adult, right	3009-10
DORO® Horseshoe Pad, Adult, left	3009-11

Shown mounted to the **DORO LUCENT®** Base Unit.

PEDIATRIC VERSION

DORO LUCENT® Horseshoe Headrest ENT, Pediatric
Item no. 1101.008

Included Items	Item no.
DORO LUCENT® Horseshoe Headrest ENT, RDL w/o Gel Pads	1101.006
DORO® Horseshoe Pad, Pediatric, right	3008-10
DORO® Horseshoe Pad, Pediatric, left	3008-11



ONE BASE FITS ALL

DORO® Horseshoe Bases share the same gel pad holder design. This means that all our horseshoe gel pads can be mounted to every horseshoe base in our portfolio. The innovative design of the **DORO®** Horseshoe Base gives you the opportunity to quickly adapt these products to adult or pediatric applications by mounting the respective gel pads, ensuring the optimal set-up for each of your patients.

DORO® QR3 XTom

MRI SMALL GANTRY CT ANGIO

The DORO® QR3 XTom Cranial Stabilization System is designed to fit small gantry CTs. Adjustable Extension Arms ensure an optimal patient placement within CT scanner gantries of 32 cm / 12 inch and larger. The XTom System comes with a specifically designed torque screw driver to set pin pressure and with the DORO® XTom U-Belt, which works like a safety net and will prevent major injuries in case of head slippage, no matter the patient's head position.

DORO® QR3 XTom Cranial Stabilization System Item no. 4002.100	
Included Items	Item no.
DORO® QR3 XTom Skull Clamp	4002.001
DORO® XTom U-Belt (3 pcs)	4002.111
DORO® XTom Storage Case	4002.030
DORO® XTom Torque Screwdriver	4002.068
DORO® XTom Base Unit Parkbench	4002-10
DORO LUCENT® Disposable Skull Pins (9 pins)	1106.103

HIGH-END IMAGING

DORO LUCENT®

Disposable Skull Pins reduce imaging artifacts to a minimum.

PRECISE NAVIGATION

Navigation tracking device adaptors can easily be attached in close proximity to the surgical field.

A SMALL GANTRY SOLUTION


Adjustable Extension Arms ensure that the patient's head fits into gantries of 32 cm / 12 inch and larger.

EASY, SAFE AND STABLE INTERFACE

Attach DORO LUNA®, DORO COBRA® or Quick-Clamp products to the form-fitting Quick-Rail® interface.

COMPATIBLE


The DORO® QR3 XTom Cranial Stabilization System is directly mountable to all standard OR tables with side rails.

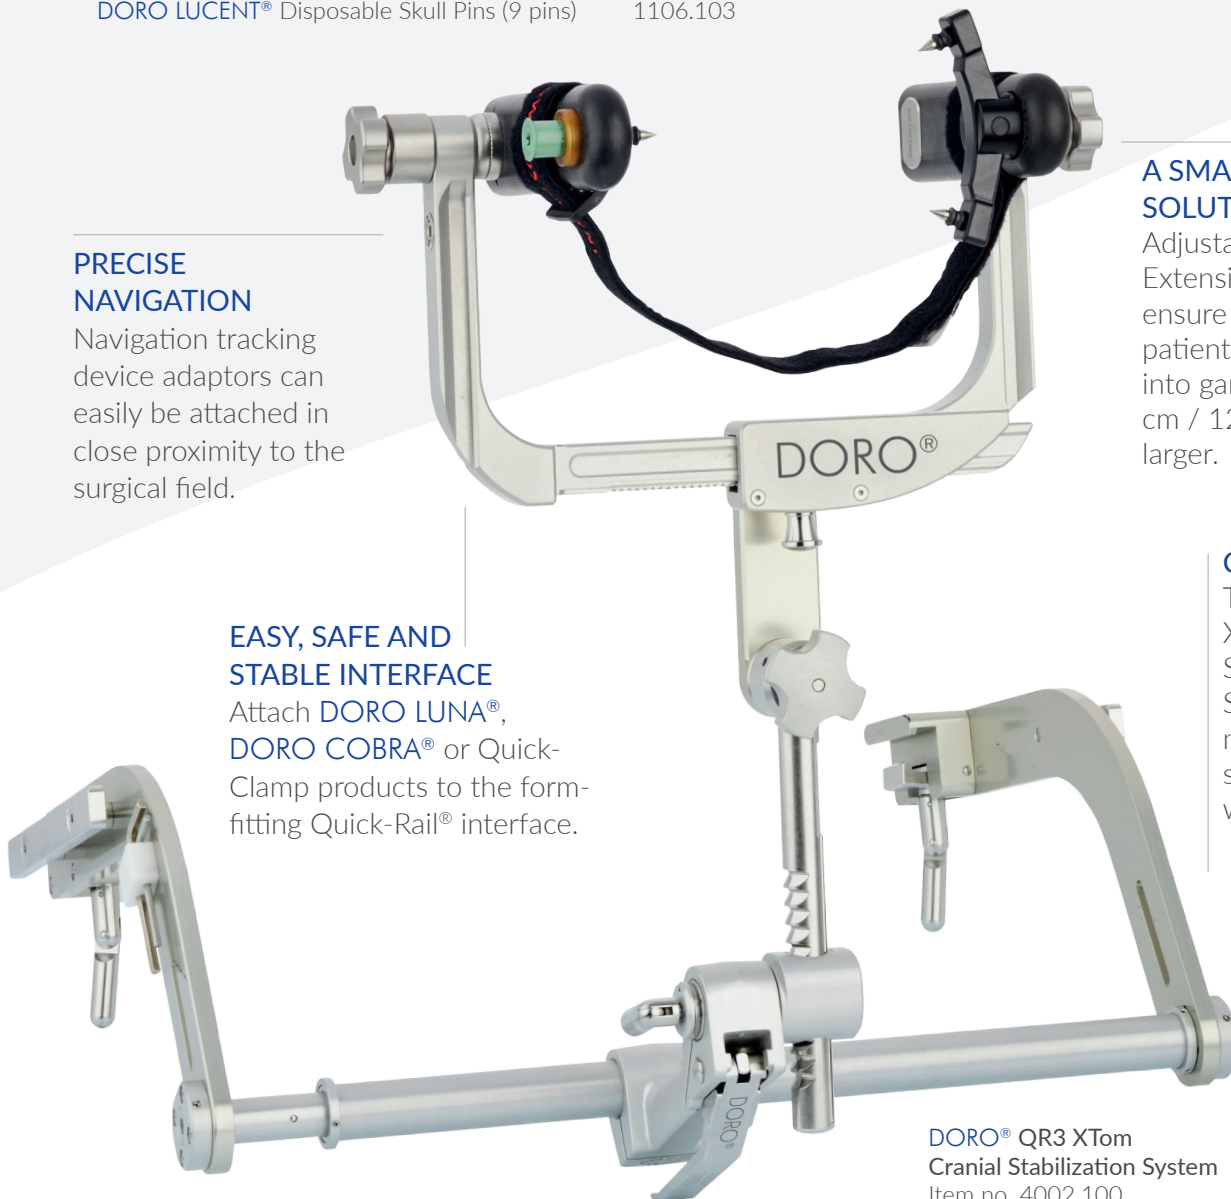

DORO® QR3 XTom
Cranial Stabilization System
Item no. 4002.100

Which DORO® System works for your Neurological scanner?


The DORO® QR3 XTom Cranial Stabilization System is designed to fit small gantry CTs like NeuroLogica's OmniTom or CereTom scanners. For CTs with larger gantries the DORO LUCENT® Headrest System is the Cranial Stabilization System of choice.

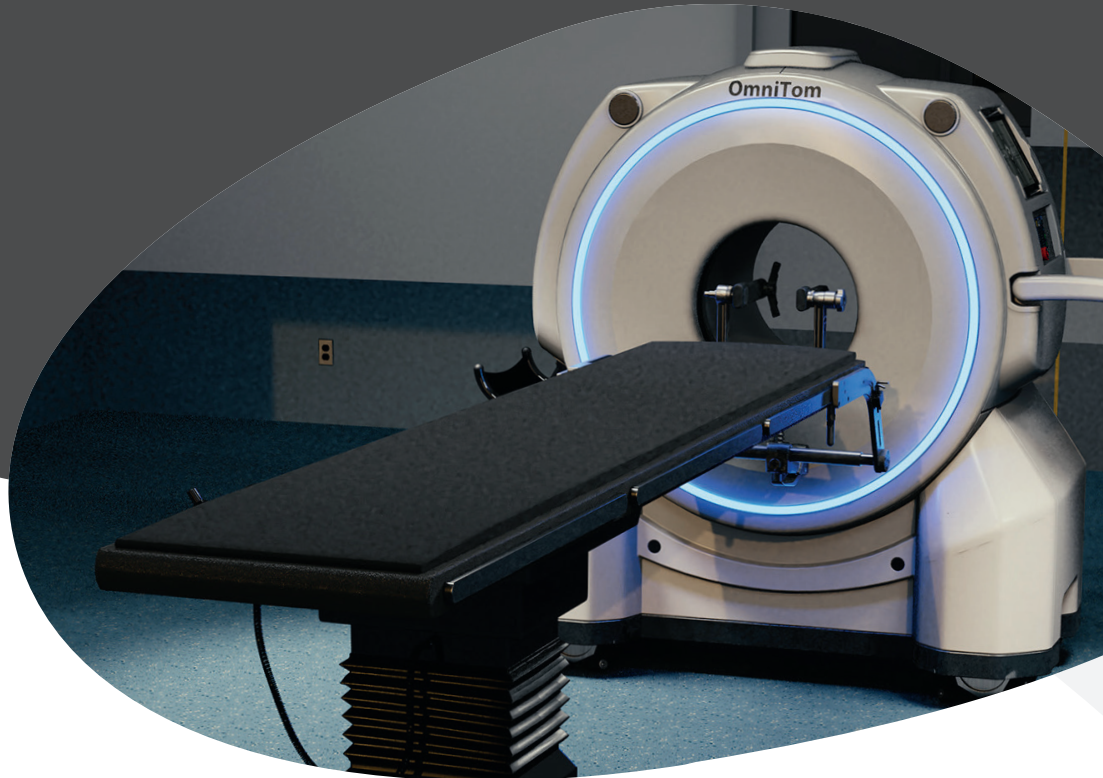

BodyTom



OmniTom



CereTom

NEUROLOGICA
SCANNER



DORO LUCENT®
Headrest System
Item no. 1101.020
(page 20)



DORO® QR3 XTom
Cranial Stabilization System
Item no. 4002.100

DORO®
SYSTEM

DORO LUCENT® iXI HEADREST SYSTEM

✓ MRI ✓ CT ✓ ANGIO

The DORO LUCENT® iXI Headrest System enhances your diagnostic capabilities by supporting intra-operative MR, CT, and Angio imaging. This allows you and your team to perform diagnostic procedures on bone and tissue during the same surgery, resulting in more precise treatment with reduced time consumption compared to separate imaging methods.

STATE-OF-THE-ART
The DORO LUCENT® iXI Headrest System is a dedicated multimodality imaging solution designed for use with MAQUET / GETINGE Magnus OR Tables and SIEMENS Nexaris Imaging Suites.



DORO LUCENT®
iXI Headrest System
Item no. 4003.500

EXTENDABLE

Quick-Rail® Technology enables you to attach accessories and retractor systems easily, quickly, and securely to the skull clamp.

FAMILIAR

The classic skull clamp design lets you apply your known routines and workflows.

MULTI-MODALITY IMAGING

Multimodality imaging is the current pinnacle of clinical, intra-operative imaging. All individual strengths of the three highend imaging modalities are combined into one versatile OR suite. This way, a surgeon is able to decide on the fly, which modality (or modalities) will benefit the patient the most, resulting in the best possible medical answer possible for each individual patient.

MRI SCANNER

SIEMENS
NEXARIS

OR TABLE

GETINGE (MAQUET)
Magnus

DORO LUCENT®
iXI Headrest System
Item no. 4003.500



Included Items	Item no.
DORO® Skull Clamp Radiolucent for DORO LUCENT® Parallelogram Adaptor	4003.001
DORO® Headplate	4003.005
DORO® Adjusting Wrench for DORO LUCENT® Parallelogram Adaptor	4003.011
DORO LUCENT® Storage Case for DORO LUCENT® Parallelogram Adaptor	4003.030
DORO LUCENT® iXI Parallelogram Adaptor	4003.511
DORO LUCENT® iXI Transfer Collision Indicator	4003.5XX
DORO LUCENT® Disposable Skull Pins, Adult (3 pcs)	1106.003

PLEASE NOTE:

With the first installation of a DORO LUCENT® iXI Headrest System, an expert training is mandatory (page 32). Please contact your local DORO® representative for details.



AN OPTIMIZED WORKFLOW

Position the patient as required for surgery before starting the actual pinning procedure with the DORO LUCENT® Headplate. This makes further movements of the sedated patient unnecessary, resulting in reduced procedural risk, less stress for the patient and increased convenience for you and your team.

The DORO LUCENT® Headplate is included in every DORO LUCENT® iXI or iMRI system.

DORO LUCENT® iMRI HEADREST SYSTEMS

MRI CT ANGIO

Solutions for Fixed MRIs

DORO LUCENT® iMRI Headrest Systems for rigidly installed MRIs are mounted to the OR table's transfer board by utilizing the DORO LUCENT® iMRI Parallelogram Adaptor, giving you the freedom you need to properly position patients for surgery. These systems are available for a variety of OR table and MRI scanner combinations. Please refer to the adjacent chart to find a product that fits your OR environment.

FAMILIAR

The classic 3-pin skull clamp design with ratcheting system allows you to rely on your trained routine and known workflows.

HIGH-END IMAGING DORO LUCENT®


Disposable Skull Pins are perfectly stable and reduce imaging artifacts to a minimum (page 16).

FAST

Directly mountable to transfer boards of selected OR table manufacturers.

FLEXIBLE

The parallelogram design supports you in positioning your patient properly for surgery.

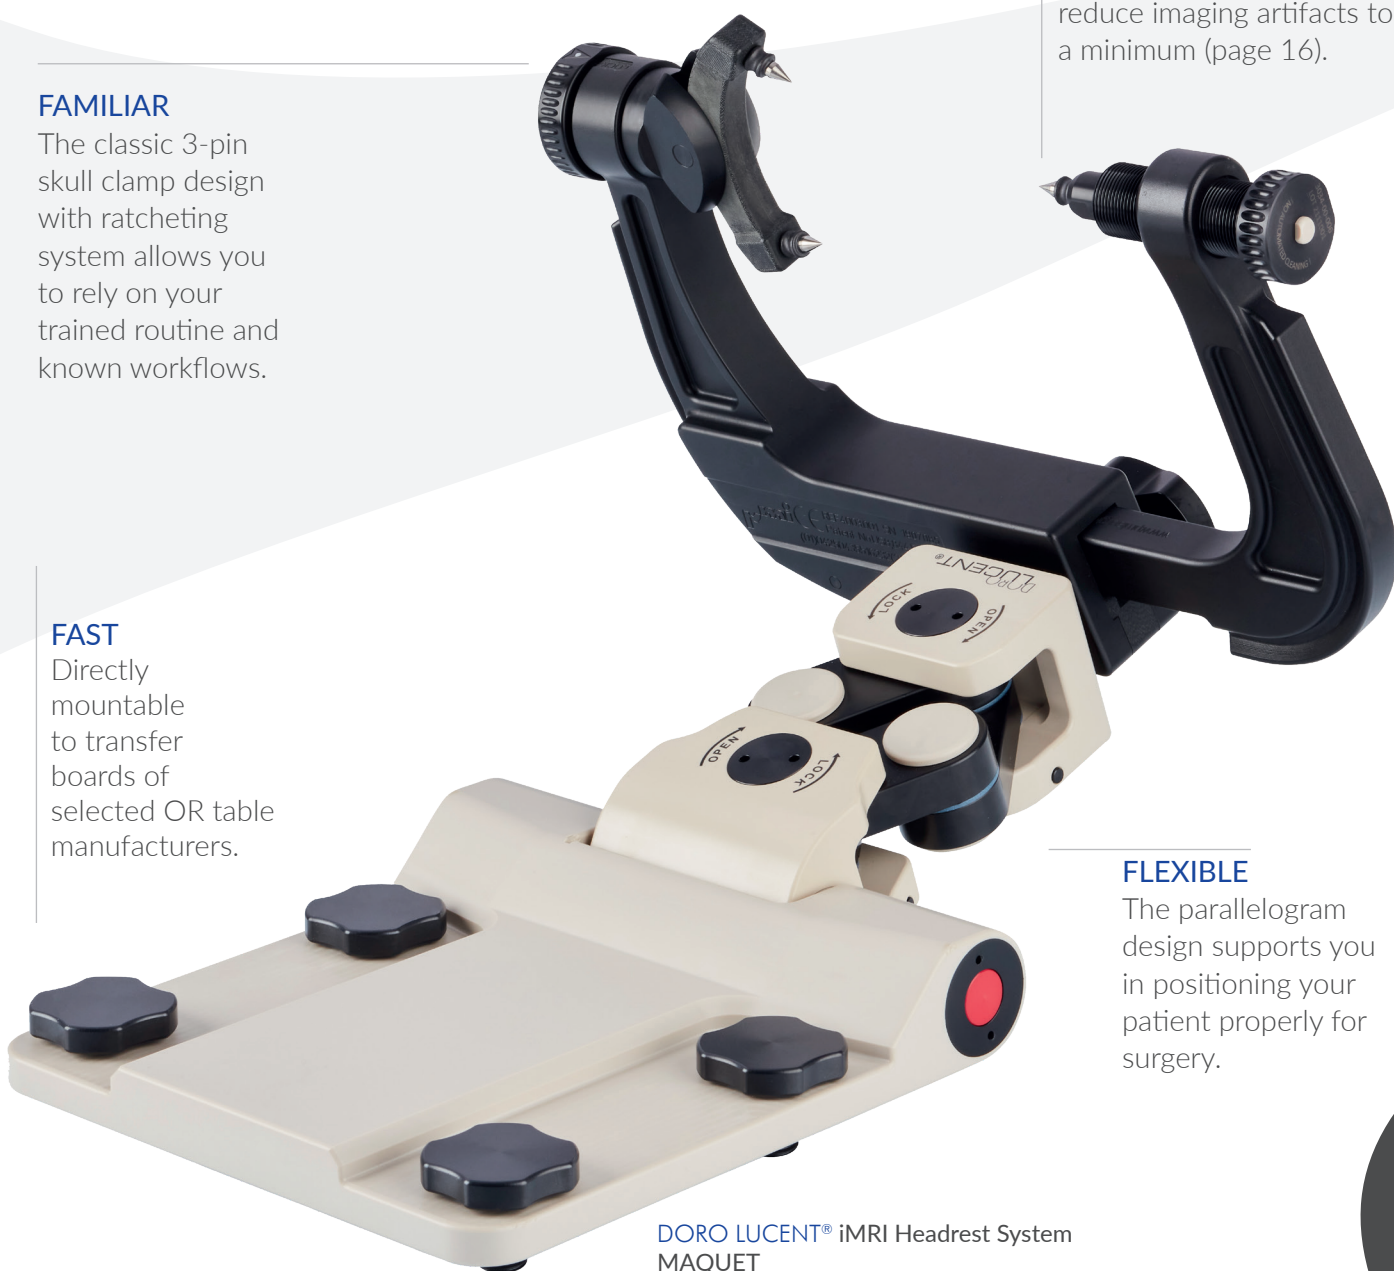

DORO LUCENT® iMRI Headrest System
MAQUET
Item no. 4003.300

MRI SCANNER

PHILIPS
Ingenia MR-OR (1.5T & 3T)

GE
3.0T Signa HDxt / Signa Artist
& Architect / Optima MR450w/
Discovery MR750 & 750w

**SIEMENS
MAGNETOM**
Aera / Skyra
Sola / Vida

**SIEMENS
MAGNETOM**
Aera / Skyra

OR TABLE
with Transfer Table Top

MIZUHO

GETINGE (MAQUET)
Alphamaquet & Otesus / Magnus

Baxter (Trumpf/Hill-Rom)
TruSystem



DORO LUCENT®
iMRI Headrest System MIZUHO
Item no. 4003.350

Included Items	Item no.
DORO® Skull Clamp Radiolucent for DORO LUCENT® Parallelogram Adaptor	4003.001
DORO® Headplate	4003.005
DORO® Adjusting Wrench for DORO LUCENT® Parallelogram Adaptor	4003.011
DORO LUCENT® Storage Case for Parallelogram Adaptors	4003.030
DORO LUCENT® iMRI Parallelogram Adaptor MAQUET	4003.311
DORO LUCENT® Disposable Skull Pins, Adult (3 pcs)	1106.003

A fitting iMRI Transfer Collision Indicator must be purchased from Phillips.

DORO LUCENT®
iMRI Headrest System MAQUET
Item no. 4003.300

Included Items	Item no.
DORO® Skull Clamp Radiolucent for DORO LUCENT® Parallelogram Adaptor	4003.001
DORO® Headplate	4003.005
DORO® Adjusting Wrench for DORO LUCENT® Parallelogram Adaptor	4003.011
DORO LUCENT® Storage Case for Parallelogram Adaptors	4003.030
DORO LUCENT® iMRI Parallelogram Adaptor MAQUET	4003.311
DORO LUCENT® iMRI Transfer Collision Indicator	4003.XXX
DORO LUCENT® Disposable Skull Pins, Adult (3 pcs)	1106.003

PLEASE NOTE:


With the first installation of a **DORO LUCENT®** iMRI Headrest System, an expert training is mandatory (page 32). Please contact your local **DORO®** representative for details.

DORO LUCENT®
iMRI Headrest System TRUMPF
Item no. 4003.200

Included Items	Item no.
DORO® Skull Clamp Radiolucent for DORO LUCENT® Parallelogram Adaptor	4003.001
DORO® Headplate	4003.005
DORO® Adjusting Wrench for DORO LUCENT® Parallelogram Adaptor	4003.011
DORO LUCENT® Storage Case for Parallelogram Adaptors	4003.030
DORO LUCENT® iMRI Parallelogram Adaptor TRUMPF	4003.211
DORO LUCENT® iMRI Pad TRUMPF	4003.212
DORO LUCENT® iMRI Transfer Collision Indicator	4003.XXX
DORO LUCENT® Disposable Skull Pins, Adult (3 pcs)	1106.003
DORO® Torx Screwdriver T45, nonmagnetic	3033-68

MOVEMENT CAPABILITIES

DORO LUCENT® Parallelogram Adaptors allow you to shift, tilt, angle and rotate the skull clamp to find a fitting position for your patient.

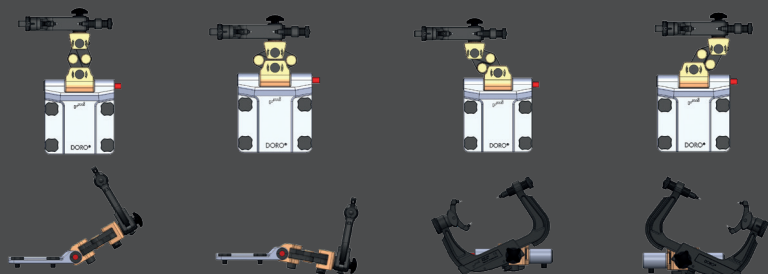

DORO LUCENT® iMRI HEADREST SYSTEMS

MRI CT ANGIO

Solution for Moving MRIs

The DDORO LUCENT® iMRI Cranial Stabilization Set IMRIS is a lightweight and intuitive intraoperative solution designed for the IMRIS Invision™ Surgical Theatre, featuring a ceiling-mounted, movable MRI. It can be quickly and easily mounted using the DORO LUCENT® iMRI Interface Adaptor. The interface to the IMRIS coil can be continuously adjusted, allowing for precise positioning.

CONVENIENT HANDLING

Proven three-point Skull Clamp and significantly more lightweight than comparable products

PLAY-FREE OPEN/LOCK

Enhanced precision for neuro-navigation

UNIQUE QUICK-RAIL®

Intuitive mounting of retractor systems or other accessories

IMPROVED FLEXIBILITY

Slim and thoughtful design allows for easy and collision-free accessibility

OPTIMIZED FOR IMRI

Continuous adjustability for precise adjustment of coil position

Minimized amount of titanium results in less artifact.



MRI SCANNER

SIEMENS
MAGNETOM
Espree / Aera
Verio / Skyra / Vida

OR TABLE

Baxter (Trumpf/Hill-Rom)
ORT 100 / 200 / 300 / 400



DORO LUCENT®
Cranial Stabilization Set IMRIS
Item no. 4003.600

Included Items	Item no.
DORO® Skull Clamp Radiolucent for DORO LUCENT® Parallelogram Adaptor	4003.001
DORO® Headplate	4003.005
DORO® Adjusting Wrench for DORO LUCENT® Parallelogram Adaptor	4003.011
DORO LUCENT® Storage Case for Parallelogram Adaptors	4003.030
DORO LUCENT® iMRI Interface Adaptor IMRIS	4003.611
DORO LUCENT® iMRI Coil Connector IMRIS	4003.631



AUTOMATIC IMAGE REGISTRATION READY


Brainlab Automatic Image Registration (AIR) is the fundamental technology for high-precision surgical navigation from start to finish. It adds intraoperatively acquired MR images to surgical navigation while maintaining the preoperative surgical plan. This updated registration compensates for potential loss of navigation accuracy during surgery.

The Brainlab registration matrix with integrated MR markers has been designed exclusively for DORO LUCENT® iMRI & iXI Headrest Systems and therefore seamlessly integrates in the standard patient positioning workflow.

DORO LUCENT® PRODUCT TRAININGS

Dedicated products like the DORO LUCENT® iMRI or iXI Headrest Systems come as a part of a larger iMRI or multimodality imaging installation. Before you start conducting live cases with these state-of-the-art products we will train you in their use. We explain functions, simulate workflows, and assist you in matching them to your distinct needs. These training sessions are held on site, in your facility, with you and your team, to offer the best possible education. DORO® application specialists will cover essential and advanced product knowledge and will match the training to your OR environment. The training will especially focus on overall system set-up & movement capabilities as well as patient positioning and clinical workflow subject to the respective imaging modality.

iMRI & iXI Product Training
Item no. 8001

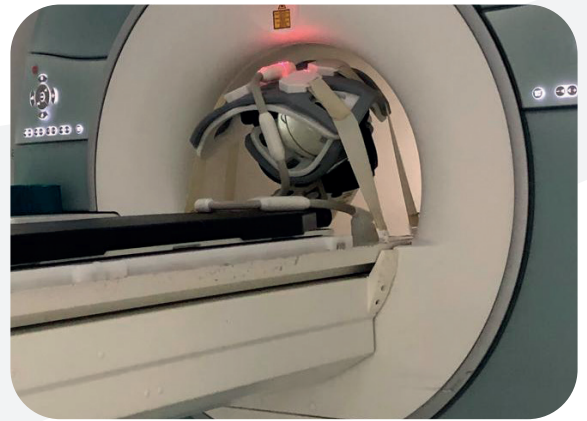

DORO LUCENT® iMRI & iXI ACCESSORIES



DORO LUCENT® Headplate
Item no. 4003.005



DORO LUCENT® iMRI Pad TRUMPF
Item no. 4003.212



DORO LUCENT® Storage Case
for Parallelogram Adaptors
Item no. 4003.030



DORO® Adjusting Wrench for
DORO LUCENT® Parallelogram Adaptor
Item no. 4003.011



DORO® Torx Screwdriver
T45, nonmagnetic
Item no. 3033-68



DORO LUCENT® iMRI
Transfer Collision Indicator
Item no. 4003.XXX



DORO LUCENT® iXI
Transfer Collision Indicator
Item no. 4003.5XX

DORO® SKULL CLAMP – SPINAL FRAMES


MRI CT ANGIO

–RADIOLUCENT –

This modification of our metal-free DORO® Skull Clamp Radiolucent is designed for spinal surgeries and can be mounted to all established spinal OR tables and spinal frames. The slim design allows the skull clamp to be lowered between the rails of the open frame, simplifying patient positioning and imaging procedures.



DORO® Skull Clamp Radiolucent for Spinal Frames shown mounted to a MIZUHO OSI Insite® table (side view).

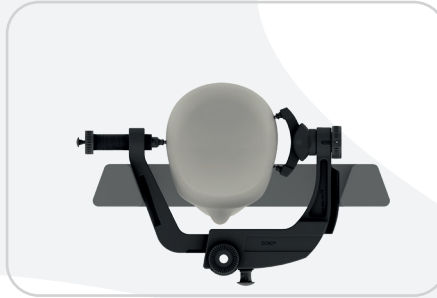

Comparison of the lowering capability of the DORO® Skull Clamp Radiolucent for Spinal Frames between the bars of an operating table for spinal surgery (front view) to the standard DORO® Skull Clamp Radiolucent.



FREEDOM IN PATIENT POSITIONING

Unique shape allows lowering of the patient's head between the rails of an open frame OR table.

VERSATILE
Quick-Rail® Technology enables you to attach accessories and retractor systems easily, quickly, and securely to the skull clamp.

DORO® Skull Clamp Radiolucent for Spinal Frames
Item no. 4004.101
(shown with DORO LUCENT® Disposable Skull Pins, page 11).

MIX & MATCH

The DORO® Skull Clamp Radiolucent can be mounted to DORO® Aluminum Swivel Adaptor and Base Unit utilizing the Mix & Match Adaptor #3033-50 (page 23) or to fitting counterparts of spinal frame table manufacturers.

DORO® OR TABLE ADAPTORS RADIOLUCENT

MRI CT ANGIO




DORO® Angiography Table Adaptor
SIEMENS, Radiolucent
for Artis Table
Item no. 4003-00



DORO® Table Adaptor
Medifa®, Radiolucent for Medifa®
OR Table 8000 & 8000 hybrid
Item no. 4004.001



DORO® Table Adaptor
STERIS, Radiolucent
for STERIS Carbon OR Tables CMAX XRAY
Item no. 4004.002

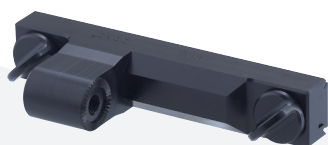

DORO® Table Adaptor
MAQUET, Radiolucent
Item no. 3031-50



DORO® Transitional Member
Radiolucent, long (160 mm)
Item no. 3032-10



DORO® Transitional Member
Radiolucent, short (120 mm)
Item no. 3032-20

For Alphamaquet 1150 and Magnus 1180
and only in conjunction with MAQUET
Adaptor, MAQUET item no. 6005.25A0.

Compatible with **DORO®** Table Adaptors
Radiolucent, item nos 3031-50,
4003-00, 4004.001, 4004.002.

Compatible with **DORO®** Table Adaptors
Radiolucent, item nos 3031-50,
4003-00, 4004.001, 4004.002.



DORO® Radiolucent Table Adaptors Set Up Possibilities

Start with the OR table manufacturer at the bottom and work your way up to the DORO® solution that works best for you.





RETRACTOR SYSTEMS

Surgeries are often connected to time-critical or stressful situations. Having to work under pressure demands the highest level of concentration. To enable you to focus on your work, we are driven to develop retractor systems which ease your workflow. Easy to set-up, convenient to use, comfortable as a hand rest, these systems will support you during the whole surgical procedure.



DORO LUNA® RETRACTOR SYSTEM

The DORO LUNA® Retractor System is made to support you in every surgery. Its open design allows you to always keep the curves parallel to the floor, independently of patient and skull clamp positioning. Tilt, shift and angle the system into any position you need and you will still be able to use the curves as a comfortable hand rest and retractor arm interface. The adaptability of the DORO LUNA® Retractor System can be further enhanced with additional accessories, making it the most versatile retractor system to date.




The DORO LUNA® Retractor System is the winner of the 2015 Freiburg Innovation Award.

CONVENIENT

Snap-on attachment of DORO COBRA® Flexible Rotary Arms on any desired position on the curve.

SUPPORTIVE

Ergonomic design makes the DORO LUNA® Curve the optimal hand support. It can be positioned parallel to the floor, independently of skull clamp position.

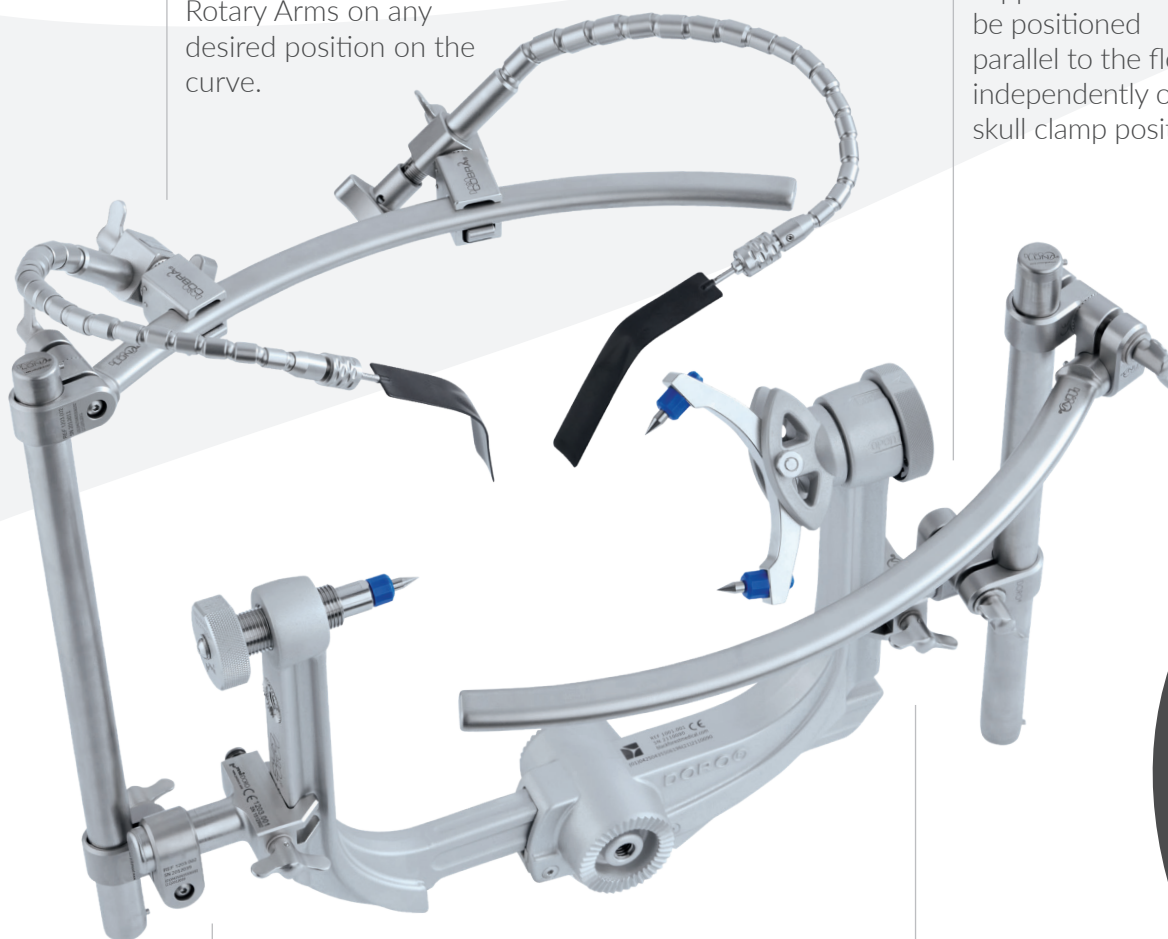

DORO LUNA®
Retractor System Standard
Item no. 1203.100
(shown mounted to the
DORO® QR3 Skull Clamp)

FAST

DORO LUNA® attaches directly to the Quick-Rail®, even over multiple layers of sterile drape.

EASY

No extra tools are needed to mount and use DORO LUNA® Retractor Systems.

DORO LUNA® Retractor System – Standard System


Item no. 1203.100

Included Items	Item no.
DORO COBRA® Flexible Rotary Arm 280mm (2 pcs)	1201.006
DORO® Retractor Sterilization Tray	1201.091
DORO LUNA® Quick-Clamp for Quick-Rail® (2 pcs)	1203.001
DORO LUNA® Coupling (4 pcs)	1203.002
DORO LUNA® Rod (2 pcs)	1203.003
DORO LUNA® Curve (2 pcs)	1203.004
DORO LUNA® Sterilization Tray	1203.091
DORO® Blade Set 102 mm, Black Coated, 5 pcs (2 sets)	3116-101

DORO LUNA® Retractor System – Compact System

Item no. 1203.200

Included Items	Item no.
DORO COBRA® Flexible Rotary Arm 280mm (2 pcs)	1201.006
DORO® Retractor Sterilization Tray	1201.091
DORO LUNA® Quick-Clamp for Quick-Rail® (2 pcs)	1203.001
DORO LUNA® Coupling (2 pcs)	1203.002
DORO LUNA® Rod	1203.003
DORO LUNA® Curve	1203.004
DORO LUNA® Sterilization Tray	1203.091
DORO® Blade Set 102 mm, Black Coated, 5 pcs (2 sets)	3116-101



GET THE BUNDLE

DORO LUNA® Standard Retractor System & DORO® QR3 Skull Clamp
Item no. 1203.110

DORO LUNA® Standard Retractor System & DORO® QR3 Headrest System
Item no. 1203.120



GET THE BUNDLE

DORO LUNA® Compact Retractor System & DORO® QR3 Skull Clamp
Item no. 1203.210


DORO LUNA® Compact Retractor System & DORO® QR3 Headrest System
Item no. 1203.220

A HIGHLY FLEXIBLE INTERFACE

Unfold the full potential of your DORO LUNA® & DORO COBRA® products by combining them in various set-ups. Mount half a DORO LUNA® Retractor System as a hand support while directly connecting DORO COBRA® Flexible Rotary Arms to the Quick-Rail® of the skull clamp, either in an imaging or in a non-imaging environment.



DORO COBRA® Retractor System mounted to the DORO® QR3 Skull Clamp.

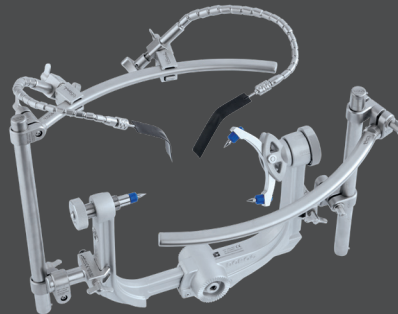


DORO LUNA® Retractor System mounted to the DORO® QR3 Skull Clamp.



DORO LUNA® & DORO COBRA® combined set-up mounted to the DORO® Skull Clamp Radiolucent.

DORO COBRA® RETRACTOR SYSTEM

The DORO COBRA® Retractor System is the retractor system of choice for minimal obstruction and access to the surgical site. DORO COBRA® Flexible Rotary Arms are directly mounted to the Quick-Rail® of either the DORO® QR3 Skull Clamp or the DORO® Skull Clamp Radiolucent. A combined set-up with DORO LUNA® components is possible and grants enhanced set-up and application possibilities.

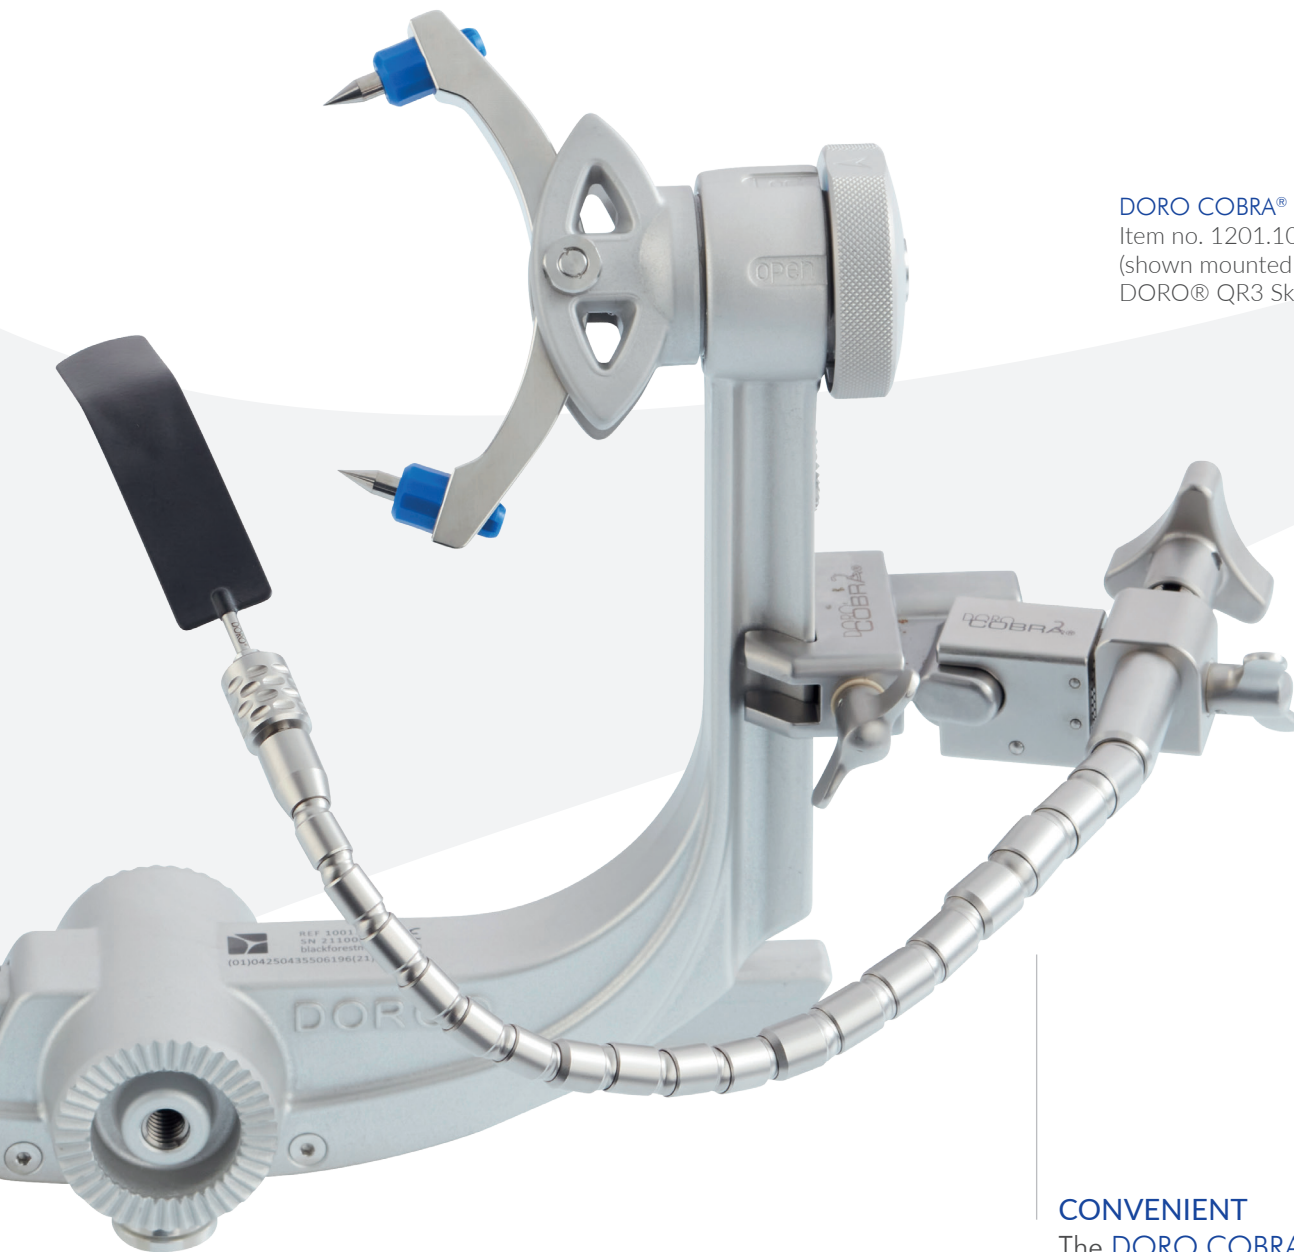

DORO COBRA® Retractor System
Item no. 1201.100
(shown mounted to the
DORO® QR3 Skull Clamp)

DORO COBRA® Retractor System for Aluminum Quick-Rail®
Item no. 1201.100

Included Items	Item no.
DORO COBRA® Quick-Clamp for Aluminum Quick-Rail® (2 pcs)	1201.021
DORO COBRA® Flexible Rotary Arm 420 mm (2 pcs)	1201.008
DORO® Blade, Black Coated, 102 x 7 mm (2 pcs)	3116-111
DORO® Blade, Black Coated, 102 x 10 mm (2 pcs)	3116-121
DORO® Retractor Sterilization Tray	1201.091

CONVENIENT

The DORO COBRA® Retractor System leaves you all the space you need to perform your surgery. You would like to use a comfortable hand support with it? Just mount a DORO LUNA® Compact Retractor System (page 39) to the other side of the skull clamp.

MIX MATCH



DORO COBRA®

Mix & Match the **DORO COBRA®** Retractor System with the **DORO®** Skull Clamp Radiolucent.

DORO COBRA® Quick-Clamp for Radiolucent Quick-Rail®
Item no. 1201.022

DORO COBRA® Retractor System for Radiolucent Quick-Rail®
Item no. 1201.109



DORO LUNA®

Mix & Match the **DORO LUNA®** Retractor System with the **DORO®** Skull Clamp Radiolucent.

DORO LUNA® Quick-Clamp for Radiolucent Quick-Rail®
Item no. 1203.009

DORO LUNA® Retractor System - Standard System for Radiolucent Quick-Rail®
Item no. 1203.109

DORO LUNA® Retractor System - Compact System for Radiolucent Quick-Rail®
Item no. 1203.209

DORO COBRA® FLEXIBLE ROTARY ARMS

DORO COBRA® Flexible Rotary Arms are smooth and very precise in their movement. Just clip them on their form-fitting counterparts like the DORO LUNA® Curve or the DORO COBRA® Quick-Clamps, mount a DORO® Brain Spatula and continue your procedure. All DORO COBRA® Retractor Arms share the ability to be quickly adjusted, even without releasing the arm's tension.



DORO COBRA® Flexible Rotary Arms

Available Items	Item no.
DORO COBRA® Flexible Rotary Arm 200 mm	1201.005
DORO COBRA® Flexible Rotary Arm 280 mm	1201.006
DORO COBRA® Flexible Rotary Arm 350 mm	1201.007
DORO COBRA® Flexible Rotary Arm 420 mm	1201.008

QUICK ADJUSTMENTS UNDER TENSION

Even under tension, repositioning of the attached brain spatula is possible. Neither the tension of the retractor arm nor the stiffness of the brain spatula will be lost while doing so.

FLEXIBLE

Four different lengths and a 360° rotational body let you position the DORO COBRA® Flexible Rotary Arms precisely at the location where you need them, gaining a high visibility on your surgical site.

FAST TO MOUNT

The snap-On technology allows to quickly, and easily mount DORO COBRA® Flexible Rotary Arms.

DORO® FLEXIBLE ARMS



DORO® Flexible Arms

Available Items	Item no.
DORO® Flexible Arm 230 mm	3114-34
DORO® Flexible Arm 300 mm	3114-35

DORO® Flexible Rotary Arms

Available Items	Item no.
DORO® Flexible Rotary Arm 200 mm	3114-36
DORO® Flexible Rotary Arm 280 mm	3114-37
DORO® Flexible Rotary Arm 350 mm	3114-38

DORO® QUICK-CLAMP

– FOR RADIOLUCENT QUICK-RAIL® –

The DORO® Quick-Clamp with Starburst for Radiolucent Quick-Rail® serves as an intuitive interface* for devices used for example in frameless stereotactic or endoscopic procedures. Designed for use over the sterile barrier and form-fittingly connected to the proven Quick-Rail® of the DORO® Skull Clamp Radiolucent, the adaptor provides a stable and secure connection point for third party devices.



**DORO® Quick-Clamp with Starburst
for Radiolucent Quick-Rail®**
Item no. 3033-69

*The interface is designed to bear a max. load of 16.8 Nm (which equals a weight of 3.4 kg attached to a horizontally mounted, 50 cm long arm). It is validated for use with the Brainlab VarioGuide™. It is the responsibility of the user to verify that third party devices can safely be secured to the DORO® Quick-Clamp with Starburst for Radiolucent Quick-Rail®. The product is shown mounted to a DORO® Skull Clamp Radiolucent.

DORO® HALO RETRACTOR SYSTEM

The DORO® Halo Retractor System features the classic halo ring design. You can easily attach it to the Quick-Rail® of DORO® QR3 Skull Clamps utilizing the DORO® Quick-Clamp or to older skull clamp versions by engaging the alternatively available C-Clamp. Rotary retractor arms, brain spatulas and accessories are available.



ADAPTABLE

Adjust the halo ring to your needs. One half ring can be angled upwards or downwards, or be removed completely.

COMPATIBLE

The DORO® Halo Retractor System fits almost all common skull clamps, either utilizing the form-fitting Quick-Rail® interface or the C-Clamp.

DORO® Quick-Clamp Halo Retractor System Item no. 1202.100T



Included Items	Item no.
DORO® Quick-Clamp Halo Coupling Set (2 pcs)	1202.010
DORO® Halo Ring	3110-01
DORO® Halo Support Rod 8 mm (2 pcs)	3110-08
DORO® Halo Universal Key (2 pcs)	3110-80
DORO® Halo Pattie Tray	3110-85
DORO® Flexible Rotary Arm 280 mm (3 pcs)	3114-37
DORO® Blade Set 102 mm, Black Coated, 5 pcs (2 sets)	3116-101
DORO® Micro Blade Set, 6 pcs	3116-20
DORO® Halo Sterilization Case w/ Rack	3117-00

DORO® Halo Retractor System w/ C-Clamp Item no. 3100-00



Included Items	Item no.
DORO® Halo Ring	3110-01
DORO® Halo Support Rod 8 mm (2 pcs)	3110-08
DORO® Halo Support Bracket w/ C-Clamp Adaptor (2 pcs)	3110-51
DORO® Halo Universal Key (2 pcs)	3110-80
DORO® Halo Pattie Tray	3110-85
DORO® Flexible Arm 230 mm (3 pcs)	3114-34
DORO® Blade Set 102mm, Black Coated, 5 pcs (2 sets)	3116-101
DORO® Micro Blade Set, 6 pcs	3116-20
DORO® Halo Sterilization Case w/ Rack	3117-00

DORO® RETRACTOR ACCESSORIES



DORO® Quick-Clamp
Item no. 1202.014




DORO® Quick-Clamp Coupling Universal
Item no. 1202.015



DORO® Halo Support Rod Holder
Item no. 1202.016



DORO® Quick-Clamp Halo Coupling Set
Item no. 1202.010



DORO® Quick-Clamp with Interface Mizuho-Type Retractors
Item no. 1201.045



DORO® Halo Support Bracket with C-Clamp Adaptor
Item no. 3110-51



DORO® Halo Ring
Item no. 3110-01



DORO® Halo Support Rod 8mm
Item no. 3110-08



DORO® Clamp Body for Skin Hooks
Item no. 3114-53



DORO® Halo Pattie Tray
Item no. 3110-85



DORO® Halo Universal Key
Item no. 3110-80



DORO® Mini Vice
Item no. 3114-54


DORO® STERILIZATION TRAYS

DORO® Sterilization Trays

Included Items	Item no.
DORO® Retractor Sterilization Tray (shown)	1201.091
DORO LUNA® Sterilization Tray (shown)	1203.091
DORO® Halo Sterilization Case w/ Rack	3117-00



DORO® MICRO BLADES

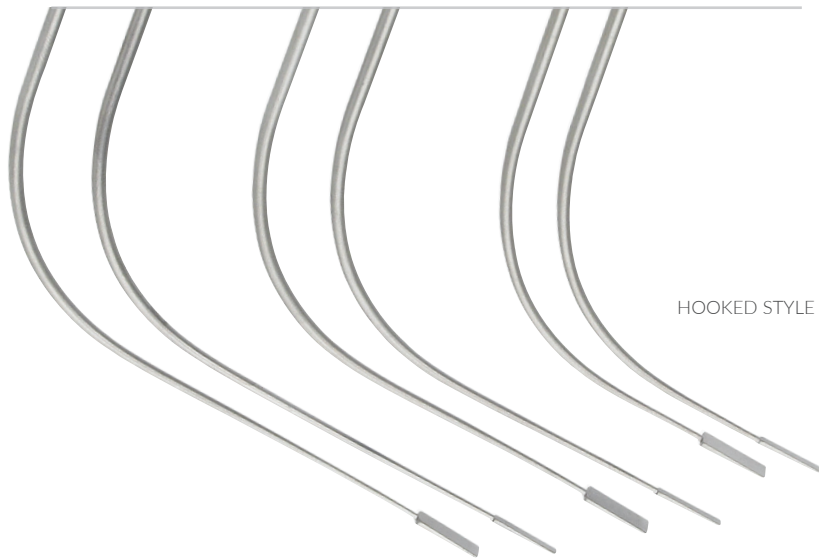

HOOKED STYLE

**DORO® Micro Blade Set,
Straight, 6 pcs.**
Item no. 3116-20



Included Items	Item no.
124 x 2 mm	3116-21
124 x 4 mm	3116-22
150 x 2 mm	3116-23
150 x 4 mm	3116-24
165 x 2 mm	3116-25
165 x 4 mm	3116-26




STRAIGHT STYLE

**DORO® Micro Blade Set,
Hooked, 6 pcs.**
Item no. 3116-40



Included Items	Item no.
124 x 2 mm	3116-41
124 x 4 mm	3116-42
150 x 2 mm	3116-43
150 x 4 mm	3116-44
164 x 2 mm	3116-45
164 x 4 mm	3116-46

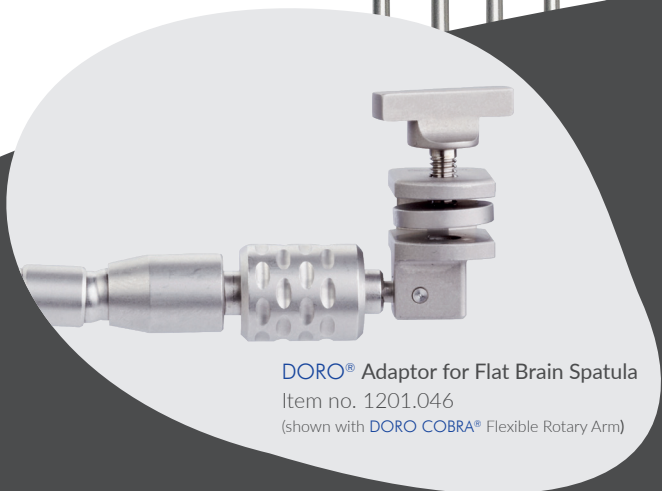

DORO® Adaptor for Flat Brain Spatula
Item no. 1201.046
(shown with **DORO COBRA®** Flexible Rotary Arm)

WANT TO USE YOUR OWN BLADES?

Do you want to use our state-of-the-art **DORO COBRA®** Flexible Rotary Arms in combination with brain spatulas you are already familiar with? The **DORO®** Adaptor for Flat Brain Spatulas is the right choice as it attaches to all **DORO®** Retractor Arms and holds all common flat brain spatulas. But try out our blades at least once... we are sure you will like them.

DORO® BLADES



DORO® Blade Set 152 mm, Black Coated, 5 pcs.
Item no. 3116-10

Included Items	Item no.
152 x 7 mm	3116-11
152 x 10 mm	3116-12
152 x 16 mm	3116-13
152 x 20 mm	3116-14
152 x 26 mm	3116-15

DORO® Blade Set 102 mm, Black Coated, 5 pcs.
Item no. 3116-101

Included Items	Item no.
102 x 7 mm	3116-111
102 x 10 mm	3116-121
102 x 16 mm	3116-131
102 x 20 mm	3116-141
102 x 26 mm	3116-151

DORO® Blade, Black Coated

not included in Set	Item no.
152 x 13 mm	3116-16
102 x 13 mm	3116-161



DORO® Blade Set 152 mm, Conical, Black Coated, 5 pcs.
Item no. 3116-60

Included Items	Item no.
152 x 2 mm	3116-61
152 x 3 mm	3116-62
152 x 4 mm	3116-63
152 x 5 mm	3116-64
152 x 6 mm	3116-65

DORO® Blade Set 102 mm, Conical, Black Coated, 5 pcs.
Item no. 3116-601

Included Items	Item no.
102 x 2 mm	3116-611
102 x 3 mm	3116-621
102 x 4 mm	3116-631
102 x 5 mm	3116-641
102 x 6 mm	3116-651



DORO® Blade Set 102 mm, Rounded Tip, Black Coated, 5 pcs.
Item no. 3116-70

Included Items	Item no.
102 x 7 mm	3116-71
102 x 10 mm	3116-72
102 x 16 mm	3116-73
102 x 20 mm	3116-74
102 x 26 mm	3116-75

CONNECTIVITY GUARANTEED
DORO® Blades and Micro Blades fit all DORO® and DORO COBRA® Retractor Arms.




WHY BLACK?

The black matt finish of our blades prevents reflections from the dazzling light focused on the surgical site during procedures and lets you concentrate on your procedure without interruptions.





www.blackforestmedical.com



DORO® REPRESENTATIVE



**BLACK
FOREST
MEDICAL
GROUP**

pro med instruments – part of Black Forest Medical Group
Headquarters | Bötzingen Straße 86 | 79111 Freiburg, Germany
Phone +49 761 384 222 10 | Email info@blackforestmedical.com

US Subsidiary | 4529 S.E. 16th Place, Suite 101 | Cape Coral, FL 33904
Toll Free 877 225 4086 | Email info.us@blackforestmedical.com

Version 13, October 2023. ©pro med instruments GmbH - part of Black Forest Medical Group. DORO®, DORO LUNA®, DORO COBRA®, DORO LUCENT® and Quick-Rail® are registered trademarks (®) of pro med instruments GmbH, Freiburg, Germany. All rights reserved. No part of this document may be reproduced in any form without written permission from copyright holder. Specifications subject to change without notice. Teflon® is a registered trademark of DuPont de Nemours GmbH. VarioGuide™ is a trademark of Brainlab. Insite® is a registered trademark of Mizuho OSI. PMT® is a registered trademark of PMT® Corporation. The information has been compiled with utmost care. Errors can, however, not be excluded. Errors do not entitle to any legal claims. We reserve the right to modify the products at any time. Please note that the present catalogue also describes products which are not approved for sale in all countries.