

IMPROVED CRANIAL STABILIZATION






SAFE PINNING ZONE¹

Staying within the indicated safe pinning zone is essential.

PIN- AND SKULL-CLAMP-POSITIONING

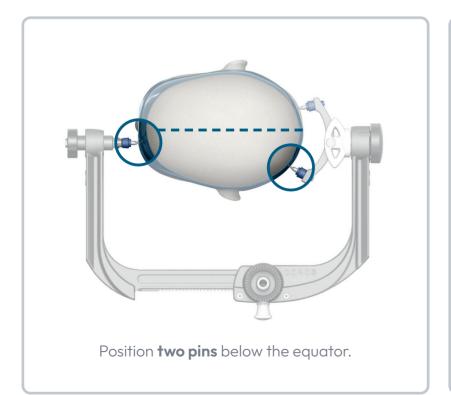




RECOMMENDED APPLICATION PINNING STEPS




Position the two-pin-holder **first**.






If vertically aligned, arrange the two-pin-holder directed upwards.

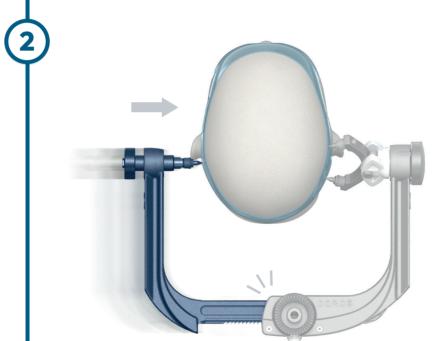

Place the contralateral single pin and push with **small force** (e.g. up to 90N | 20 lbs).

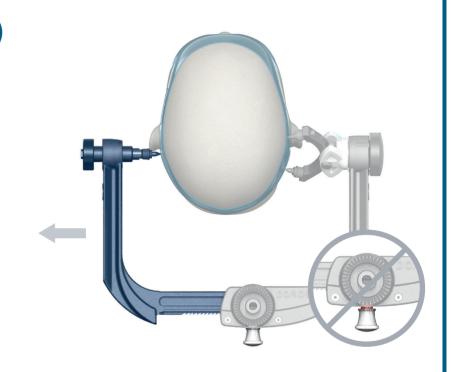

Pull with small force in the **opposite direction** to make sure that the release knob is secured.



Increase the pin force by means of the **torque screw**.



© Black Forest Medical GmbH, all rights reserved

